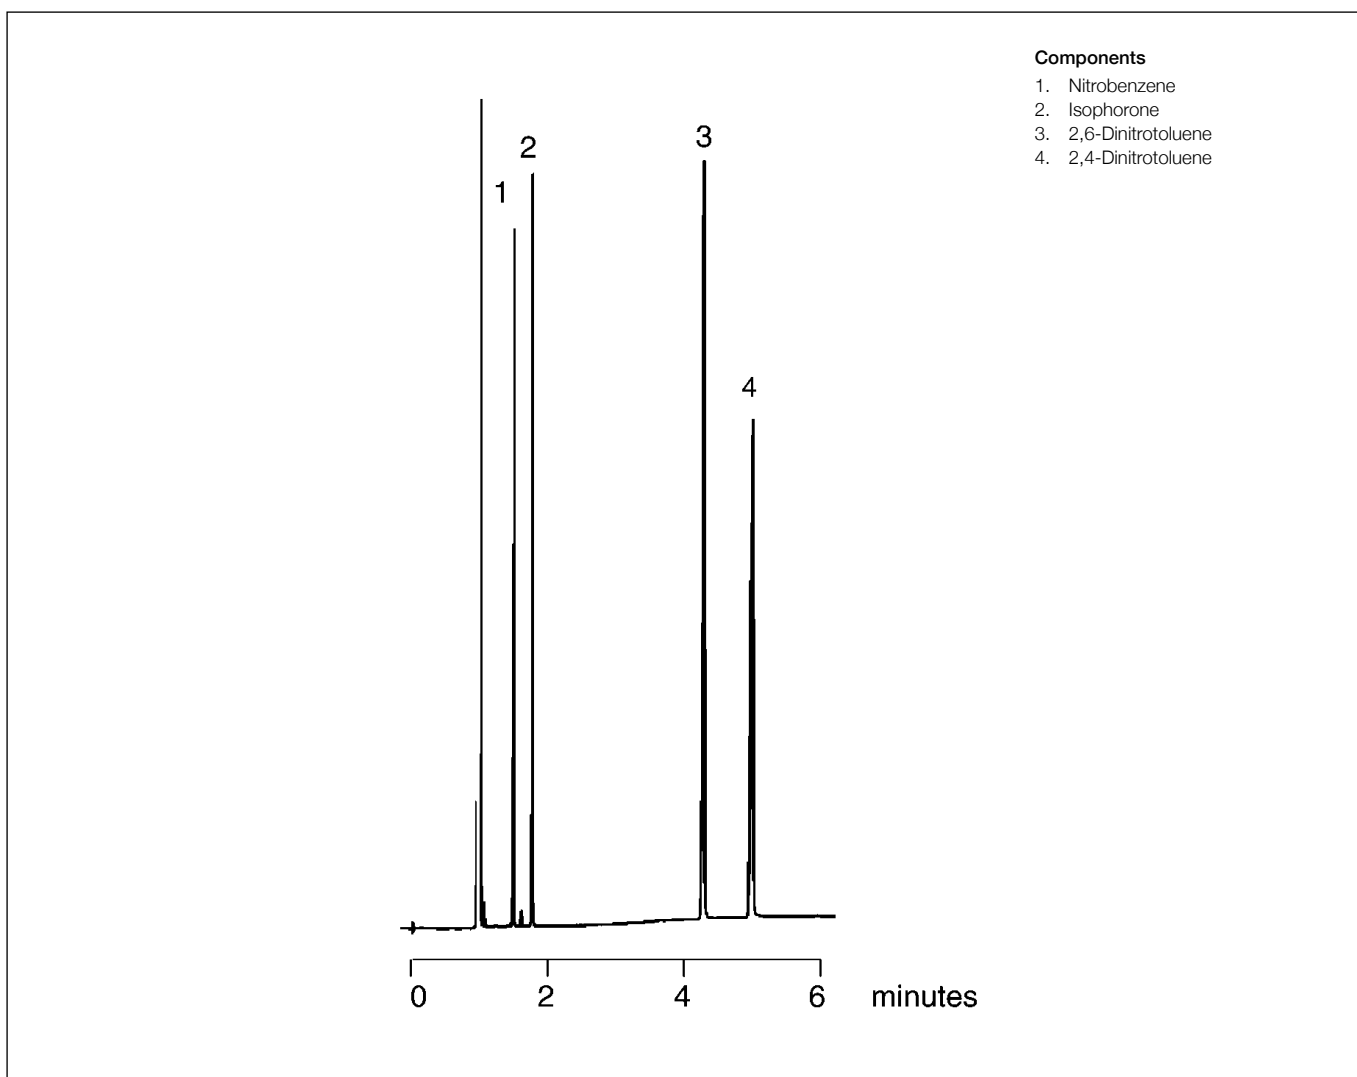


## Analysis of nitroaromatics (USEPA 609)

**BP20 (WAX)**

<b>Column part number</b>	<b>054448</b>		
Phase	BP20 (WAX)	Final temperature	240°C, 3 min
Column	12 m x 0.53 mm x 1.0 µm	Detector	FID
Initial temperature	190°C, 0 min	Injection mode	Split
Rate	15°C/min	Carrier gas	H <sub>2</sub>


 For more information visit [www.trajanscimed.com](http://www.trajanscimed.com) or contact [techsupport@trajanscimed.com](mailto:techsupport@trajanscimed.com)