

Application News

X-ray Analysis EDX-7000 / XRD-6100

Identification of Copper Concentrates Using EDX and XRD

R. Ogawa, A. Urushizaki

User Benefits

- EDX enables non-destructive and rapid qualitative analysis of constituent elements with only simple pretreatment.
- The elemental information from EDX can be utilized for XRD to identify minerals with greater accuracy.
- ◆ Since XRD can determine the compound form of an element, the accuracy of qualitative-quantitative analysis of EDX can be improved.

■ Introduction

The copper ore mined from a deposit has a copper content of about 1 %, and is refined to a copper concentrate with a grade of about 20 to 40 % through a process called ore dressing, including crushing and polishing. This copper concentrate is then smelted in a refinery to raise the copper grade to nearly 99 %.

Copper ore contains a variety of minerals other than coppercontaining minerals. Although EDX can perform qualitativequantitative analysis of elements, it cannot determine their compound forms or identify minerals. However, by combining the elemental information from EDX and database search based on X-ray diffraction, it is possible to identify minerals in copper ores and their residues after dressing and obtain useful information for the next process. In addition, the compound form information obtained from X-ray diffraction can be utilized for calculating the qualitative-quantitative results of EDX with greater accuracy.



Sample ①: EDX



Sample 2: EDX

Fig. 2 Sample Preparation

■ Samples

Fig. 1 shows two samples. Sample ① is copper concentrate powder and sample ② is residue after dressing of copper ore.



Sample ① (Copper Concentrate Powder)



Sample ② (Residue After Copper Dressing)

Fig. 1 Samples

■ Sample Preparation

As sample preparation, the powdered samples were dried by heating at 110 °C for 2 hours and then ground in a mortar to be uniform

The sample for EDX analysis was placed in a sample container lined with a 5 μm -thick polypropylene film and lightly pressed down for measurement.

The cavity of an aluminum holder for XRD was filled with powder sample and pressed to make the surface flat for measurement.

Fig. 2 shows the samples after preparation.

1. Qualitative Analysis via EDX

■ Elements

11Na to 92U

■ Results of EDX Qualitative Analysis

 $Qualitative\ analysis\ was\ conducted\ using\ EDX-7000.$

In order to obtain the elemental information necessary for qualitative analysis with XRD, a quantitative analysis was performed using the fundamental parameter (FP) method, briefly assuming the compound form to be oxides. Table 1 shows the top 10 elements contained in each sample.

Table 1 Top 10 Elements in Content

Sample name	Elements	
Sample ①	S, Fe, Zn, Cu, Si, Ca, Al, Mg, Pb, K	
Sample ②	Sample ② Si, Al, S, Fe, Mg, K, Zn, Cu, Ca, Ba	

2. Qualitative Analysis via XRD

■ Measurement with XRD

Copper-containing ores are composed of a variety of minerals. To identify such minerals, the use of an X-ray diffractometer (XRD) is effective. In this study, the powders of sample 1 and sample 2 were measured with the XRD-6100. The automatic 5-sample change stage was mounted to the XRD-6100, and the sample packed in the aluminum holder was loaded. Fig. 3 shows the appearance. Also, Table 4 shows the measurement conditions.

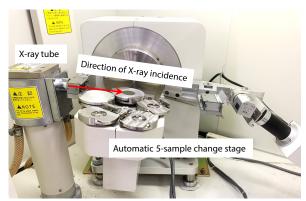


Fig. 3 Attachment and Sample Mounted on XRD-6100

X-ray Diffraction Patterns and Qualitative Analysis

Fig. 4 shows the X-ray diffraction patterns of sample 1 and sample 2.

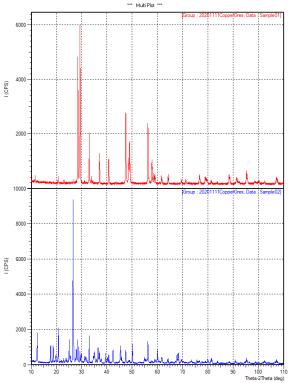
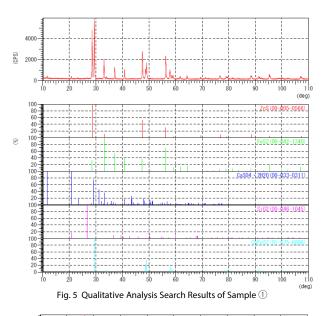


Fig. 4 X-ray Diffraction Patterns of Sample 1 (upper) and Sample 2 (lower)

In the qualitative analysis with XRD, if a database search is performed without setting the constituent elements, a large number of substances with closely similar crystal systems but composed of different elements may be returned as candidates. It is therefore important to register the appropriate elemental information in advance to obtain the correct search results.

In this study, we used the qualitative analysis results obtained by EDX (Table 1), registered them as effective elements in the qualitative analysis software, and performed a search using the ICDD (International Centre for Diffraction Data) PDF2 database.

At that time, we added H, which cannot be detected by EDX, and O, which is not used in the qualitative analysis, assuming the compound forms to be hydroxides, oxides, etc. Figs. 5 and 6 show the results of the qualitative analysis.






Fig. 6 Qualitative Analysis Search Results of Sample ②

Table 2 shows a list of the minerals contained and their simple quantitative values based on the RIR method. In sample ①, metal sulfides such as sphalerite, pyrite, and chalcopyrite were abundant, with small amounts of gypsum and quartz, a silicate mineral. In contrast, sample ② contained a large amount of silicate minerals such as quartz, clinochlore, and muscovite, as well as sulfides such as pyrite, a small amount of sphalerite, and chalcopyrite.

Table 2 List of Minerals Contained

Sample name	Component		Quantitative value (RIR method)
Sample ①	ZnS	Sphalerite	36
	FeS ₂	Pyrite	37
	CaSO₄ · 2H₂O	Gypsum	3
	SiO ₂	Quartz	1
	CuFeS ₂	Chalcopyrite	23
Sample ②	SiO ₂	Quartz	35
	FeS ₂	Pyrite	13
	ZnS	Sphalerite	4
	CuFeS ₂	Chalcopyrite	1
	(Mg, Fe, Al) ₆ (Si, Al) ₄ O ₁₀ (OH) ₈	Clinochlore	35
	KAI ₂ (Si, AI) ₄ O ₁₀ (OH) ₂	Muscovite	11

(Unit: wt%)

3. Quantitative Analysis via EDX

Figs. 7 and 8 show the results of qualitative-quantitative analysis with EDX.

From the XRD analysis results, it came out Mg, Al, Si, and K are largely contained as oxides, Fe, Cu, and Zn as sulfides, and

Ca as a sulfate. We therefore performed quantitative analysis based on the EDX measurement results mentioned above, using the FP method, assuming the compound forms of Mg, Al, Si, and K to be oxides.

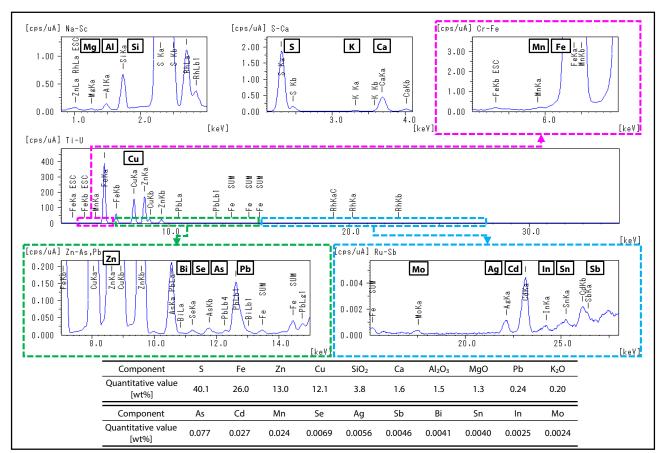


Fig. 7 Results of Qual-Quantitative Analysis of Sample ①

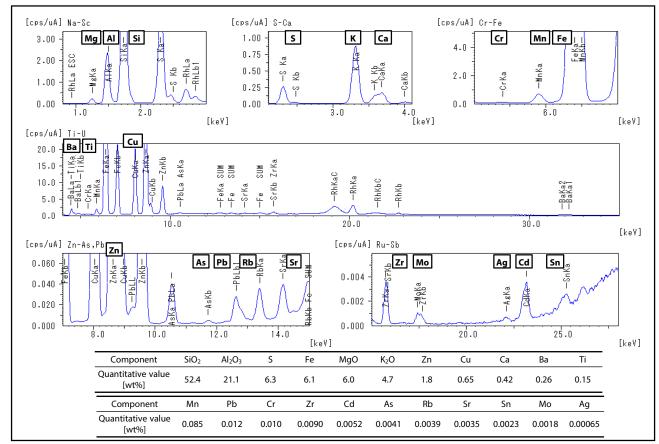


Fig. 8 Results of Qual-Quantitative Analysis of Sample $\ensuremath{@}$

■ Measurement Conditions

Table 3 EDX Measurement Conditions

Instrument	: EDX-7000
Elements	: Na-U
Analysis group	: Qualitative analysis and quantitative analysis
Detector	: SDD
X-ray tube	: Rh target
Tube voltage	: 50 [kV] (Ti-U) (Cr-Fe) (Zn-As, Pb) (Ru-Sb),
	15 [kV] (Na-Sc) (S-Ca)
Tube current	: Auto [μA]
Collimator	: 10 [mmφ]
Primary filter	: Non (Ti-U) (Na-Sc), #2 (S-Ca), #3 (Cr-Fe),
	#4 (Zn-As, Pb), #1 (Ru-Sb)

Atmosphere : Vacuum Integration time : 60 [s] x 6 Ch Dead time : Max. 30 [%]

> Table 4 Measurement Conditions for Qualitative Analysis with X-ray Diffractometer

Instrument : XRD-6100 X-ray tube : Cu target Kβ cut : Counter monochromator Detector : Scintillation detector Attachment : Automatic 5-sample change stage Voltage - current : 40 kV-40 mA

Slit condition : DS=1°, SS=1°, RS=0.3 mm Measurement mode : θ -2 θ continuous scan

Measurement speed : 2°/min Measurement step : 0.02° Measurement angle range : θ -2 θ =10-110° Rotation : 60 rotations/min

■ Conclusion

The copper ores before and after dressing were analyzed to determine the composition and compound forms with EDX and

By using the elemental information obtained from the qualitative analysis with EDX, a more accurate XRD database search became possible. Furthermore, more accurate quantitative analysis with EDX also became possible by taking into account the compound form obtained from qualitative analysis with XRD.

From these results, it was found that utilizing the results of both EDX and XRD as preliminary information was effective to analyze copper ore before and after dressing.

<References>

- K. Tomita: Industrial Raw Materials Dressing Handbook, Kyoritsu Shuppan (1966)
- H. Sekiguchi: Some Applications of Automated Fundamental X-ray Diffraction Techniques, Shimadzu Review Vol.52 [2] (1995)



Shimadzu Corporation

Analytical & Measuring Instruments Division Global Application Development Center

www.shimadzu.com/an/

For Research Use Only. Not for use in diagnostic procedures.
This publication may contain references to products that are not available in your country. Please contact us to check the availability of these

products in your country.

The content of this publication shall not be reproduced, altered or sold for any commercial purpose without the written approval of Shimadzu. See http://www.shimadzu.com/about/trademarks/index.html for details.

Third party trademarks and trade names may be used in this publication to refer to either the entities or their products/services, whether or not they

The information contained herein is provided to you "as is" without warranty of any kind including without limitation warranties as to its accuracy or completeness. Shimadzu does not assume any responsibility or liability for any damage, whether direct or indirect, relating to the use of this publication. This publication is based upon the information available to Shimadzu on or before the date of publication, and subject to change . without notice.

First Edition: Jun. 2021

01-00104-EN