



Chromatography columns and consumables  
**Pharma workflow solutions**

# Complete pharma workflow solutions

For pharma scientists pursuing great understanding of quality control and impurity regulation the correct workflow selection – from when the sample enters the lab until the sample is analyzed – can be imperative for their results.

We strive to create a better understanding of how to compose an optimal workflow allowing scientists to improve their method and resolve more, even save time and solvent, while staying within government regulations. The workflows in this brochure represent a fraction of available solutions from Thermo Fisher Scientific.

For more information or other workflows, please [contact us](#).

## Discovery DMPK

- Thermo Scientific™ HyperSep™ protein precipitation plates
- Thermo Scientific™ Accucore™ (U)HPLC columns
- Thermo Scientific™ Acclaim™ C18 (U)HPLC columns
- Thermo Scientific™ Titan3™ syringes
- Thermo Scientific™ WebSeal™ well plates and mats

## Development DMPK/Pre-clinical



- Thermo Scientific™ SOLA™/SOLA $\mu$  SPE plates and cartridges
- Thermo Scientific™ HyperSep™ SPE cartridges and plates
- Accucore (U)HPLC columns
- Thermo Scientific™ Hypersil GOLD™ (U)HPLC columns
- WebSeal well plates and mats

## Clinical

- SOLA/SOLA $\mu$  SPE plates and cartridges
- Accucore (U)HPLC columns
- Hypersil GOLD (U)HPLC columns
- WebSeal well plates and mats

## QA/QC

- Accucore (U)HPLC columns
- Hypersil GOLD (U)HPLC columns
- Thermo Scientific™ TraceGOLD™ GC columns
- Titan3 syringe syringes
- Thermo Scientific™ SureSTART™ vials and caps

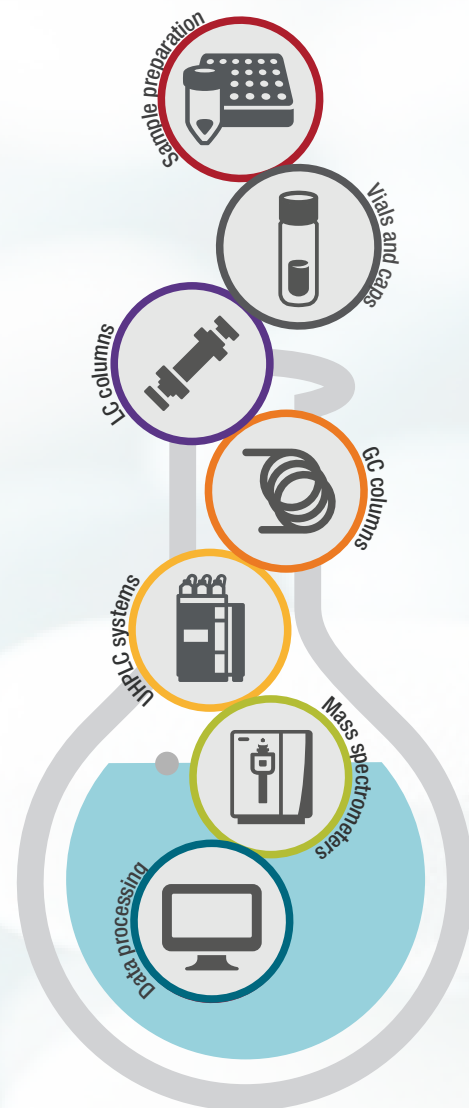

Want to make sure you choose the right columns? Use our selection guide



Want to make sure you choose the right vial for your analysis? Use our SureSTART selection guide

# Contents

## Pharma workflow solutions

---

|                              |   |
|------------------------------|---|
| ● Nitrosamine workflow       | 4 |
| ● Ibuprofen workflow         | 5 |
| ● Cepha antibiotics workflow | 6 |
| ● Solvent residue workflow   | 7 |

---

## Learn how to modernize your method

---

## Featured products

---

|                                |    |
|--------------------------------|----|
| ● HPLC columns and accessories | 9  |
| ● GC columns                   | 11 |
| ● GC accessories               | 12 |
| ● Vials and caps               | 13 |

---

# Nitrosamine workflow

## Great peak capacity method on Acclaim PA2 columns

A rapid, highly selective, and sensitive method was developed using Thermo Scientific™ Acclaim™ Polar Advantage II (PA2) column, Thermo Scientific™ Vanquish™ Horizon UHPLC system, and the Thermo Scientific™ Orbitrap Exploris™ 120 mass spectrometer for detection and quantitation of nine nitrosamines in commercially available ranitidine drug products. By combining the robust and reproducible chromatography with the 120,000 mass resolving power, fast scanning speed, and sub-ppm mass accuracy of the Orbitrap Exploris 120 system, the resultant method can provide reliable and confident quantitation of nine nitrosamine impurities that meet the September 2020 U.S. FDA regulatory acceptance limits.

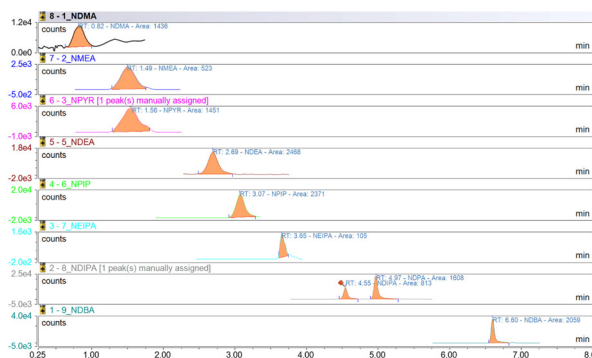


Figure 1. XIC of quantitation ion of nitrosamine impurities in 0.5 ng/mL check standard at a mass tolerance setting of 3 ppm

**Application note:** HRAM liquid chromatography mass spectrometry (LC-MS) method for the determination of nitrosamine impurities in drugs



Vanquish Horizon UHPLC system



Orbitrap Exploris 120 mass spectrometer



Acclaim PA2 column



Acclaim guard holder and coupler



SureSTART vial and cap

### Workflow solution

| Thermo Scientific instruments                          | Cat. no.                          |
|--|-----------------------------------|
| Vanquish Horizon UHPLC system                          | <a href="#">IQLAAAG-AFAPUMZZZ</a> |
| Orbitrap Exploris 120 mass spectrometer                | <a href="#">BRE725531</a>         |
| Thermo Scientific columns and guard columns            | Cat. no.                          |
| Acclaim PA2 column                                     | <a href="#">068990</a>            |
| Acclaim PA2 guard cartridge                            | <a href="#">069692</a>            |
| Thermo Scientific™ Acclaim™ guard holder and coupler   | <a href="#">069707</a>            |
| Thermo Scientific vials and caps                       | Cat. no.                          |
| Thermo Scientific™ SureSTART™ 1.5 mL screw vial        | <a href="#">6PSV9-TR1</a>         |
| Thermo Scientific™ SureSTART™ 9 mm screw cap           | <a href="#">6PSC9ST1</a>          |
| This workflow includes the newest recommended products |                                   |

[Find out more about nitrosamine impurity analysis](#)



**Confidently detect and quantify genotoxic impurities**

Nitrosamine impurities analysis solution guide



**Featured nitrosamine solutions**

We're here for you each step of the way...

# Ibuprofen workflow

## Fast and reliable method on Accucore C18 columns

The Thermo Scientific™ Accucore™ C18 column demonstrates excellent performance for the analysis of ibuprofen with minimal peak tailing. The analytical results exceeded the specifications stated in the United States Pharmacopeia (USP) monograph and there was excellent reproducibility between runs. The Accucore C18 columns are therefore an excellent choice for the analysis of ibuprofen and valerophenone.

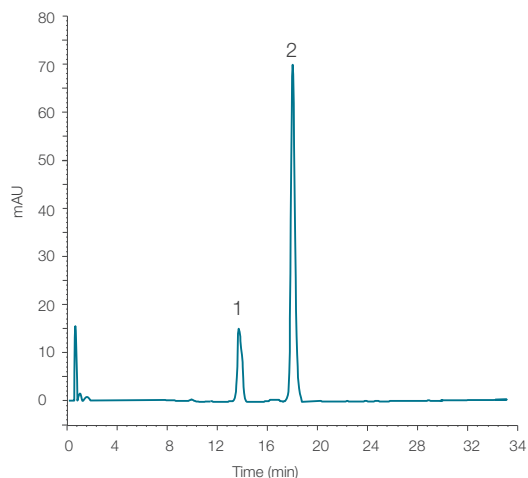


Figure 2. Improved analysis of ibuprofen and valerophenone using a Accucore C18 column

[AppsLab library](#): Improved analysis of ibuprofen and valerophenone using Accucore C18 column



Vanquish Core HPLC system



Accucore C18 column



Uniguard direct-connection guard cartridge holder



SureSTART vial and cap

### Workflow solution

| Thermo Scientific instrument  | Cat. no.                        |
|---|---------------------------------|
| Thermo Scientific™ Vanquish™ Core HPLC system                         | <a href="#">VQ-CORE-QUAT-01</a> |
| UV detector   |                                 |
| Thermo Scientific columns and guard columns                           | Cat. no.                        |
| Accucore C18 column   | <a href="#">17126-104630</a>    |
| Accucore C18 guard cartridge  | <a href="#">17126-014005</a>    |
| Thermo Scientific™ Uniguard™ direct-connection guard cartridge holder | <a href="#">850-00</a>          |
| Thermo Scientific vials and caps                                      | Cat. no.                        |
| Thermo Scientific™ SureSTART™ 2 mL screw vial                         | <a href="#">6ASV9-1P</a>        |
| Thermo Scientific™ SureSTART™ 9 mm screw cap                          | <a href="#">6ASC9ST1</a>        |
| This workflow includes the newest recommended products                |                                 |



**Want to make sure you choose the right vial for your analysis?** Use our SureSTART selection guide

# Cepha antibiotics workflow

## Improved peakshape with Hypersil GOLD columns

Hypersil GOLD columns are exceptionally reproducible for reliable chromatography, column after column. This allows the user to be confident that assays developed with the Hypersil GOLD columns will be robust and stable for the life of the assay. Golden features of Hypersil GOLD is the outstanding peak shape that results in greater sensitivity. When peaks exhibit tailing, peak height is reduced, therefore compromising the sensitivity of the analysis. The highly symmetrical peaks provided by Hypersil GOLD columns enhance peak height and allow for optimised peak integration calculations. This can be particularly critical when low concentrations of an analyte are present, for example in an impurity assay.

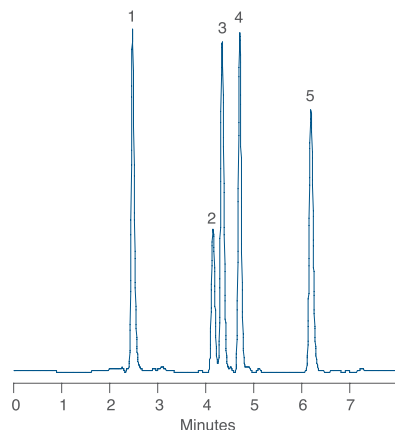


Figure 3. Cepha antibiotics

**Brochure:** [Hypersil GOLD HPLC columns](#). Outstanding peak shape for your separations



Vanquish Core  
HPLC system



Hypersil GOLD  
column




Uniguard  
direct-connection  
guard cartridge holder



SureSTART  
vial and cap

### Workflow solution

| Thermo Scientific instrument                           | Cat. no.                        |
|--|---------------------------------|
| Vanquish Core HPLC system                              | <a href="#">VQ-CORE-QUAT-01</a> |
| UV detector  |                                 |
| Thermo Scientific columns and guard columns            | Cat. no.                        |
| Hypersil GOLD column                                   | <a href="#">25005-154630</a>    |
| Hypersil GOLD guard cartridge                          | <a href="#">25005-014001</a>    |
| Uniguard direct-connection guard cartridge holder      | <a href="#">850-00</a>          |
| Thermo Scientific vials and caps                       | Cat. no.                        |
| SureSTART 2 mL glass screw vial                        | <a href="#">6ASV9-1P</a>        |
| SureSTART 9 mm screw cap                               | <a href="#">6ASC9ST1</a>        |
| This workflow includes the newest recommended products |                                 |




**Want to make sure you  
choose the right columns?**  
Use our selection guide

# Solvent residue workflow

## Expected separations on TraceGOLD columns

Organic solvents are widely used in the synthesis of pharmaceutical products and cannot always be completely removed during the manufacturing processes. To ensure safety, final products are tested to assess whether the solvents used during the manufacturing processes have been efficiently removed or, if still present, their concentration is within the accepted limits. The Thermo Scientific™ TraceGOLD™ TG-624 column allows to easily meet and exceed USP method resolution requirement ( $R_s \geq 1.0$ ), delivering expected chromatographic separation. And in pair with the Thermo Scientific™ TraceGOLD™ TG-WaxMS GC column the full requirement of the monograph is met.

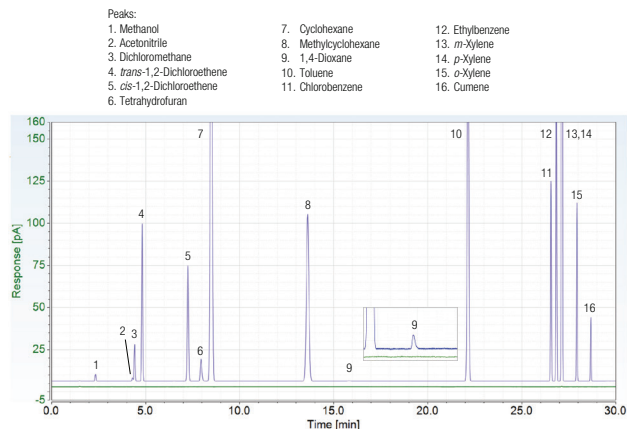

**Figure 4. Comparison between Class 2A standard solution (blue) and acetylsalicylic solution (green).** Criteria are met as no residual solvent peaks could be detected in the test sample.

**Application note:** Routine-grade performance of a new static headspace autosampler for the analysis of residual solvents according to USP <667> method



TRACE 1600 gas chromatograph with TriPlus system



TraceGOLD column



Super Clean gas cartridge filter



SureSTART vial and cap

### Workflow solution

| Thermo Scientific instrument   | Cat. no.                       |
|--|--------------------------------|
| Thermo Scientific™ TRACE™ 1600 gas chromatograph with Thermo Scientific™ TriPlus™ system | <a href="#">MI-148000-0001</a> |
| Thermo Scientific GC columns and guard columns   | Cat. no.                       |
| TraceGOLD TG-624, TG-624SiMS GC columns  | <a href="#">26059-3390</a>     |
| TraceGOLD TG-WaxMS GC column   | <a href="#">26088-1430</a>     |
| Thermo Scientific™ GuardGOLD™ capillary column   | <a href="#">26050-0532</a>     |
| Thermo Scientific GC accessories   | Cat. no.                       |
| Thermo Scientific™ ferrule   | <a href="#">290VA192</a>       |
| Thermo Scientific™ nut   | <a href="#">35050458</a>       |
| Thermo Scientific™ Super Clean™ gas cartridge filter with base                           | <a href="#">60180-830</a>      |
| Super Clean gas cartridge filters  | <a href="#">60180-824</a>      |
| Thermo Scientific vials and caps   | Cat. no.                       |
| Thermo Scientific™ SureSTART™ 20 mL crimp vials  | <a href="#">6ACV20-1R</a>      |
| Thermo Scientific™ SureSTART™ 20 mm crimp cap  | <a href="#">6PBCC20-ST3</a>    |
| This workflow includes the newest recommended products                                   |                                |




**Want to make sure you choose the right vial for your analysis?** Use our SureSTART selection guide

# Learn how to modernize your method

## Reduce time and solvent usage with newer technology columns

By modernizing an older USP monograph after the regulation provided in USP 621 you can reduce the run time and reduce solvent consumption greatly by migrating from a 5 µm to a 3 µm column. Moving to a UHPLC column will further increase time and solvent saving. The new US Pharmacopeia revision, due to release on December 1<sup>st</sup>, 2022, allows for modernization of both isocratic and gradient method. An example of the modernization of for organic impurities of Pramipexole dihydrochloride is shown below.

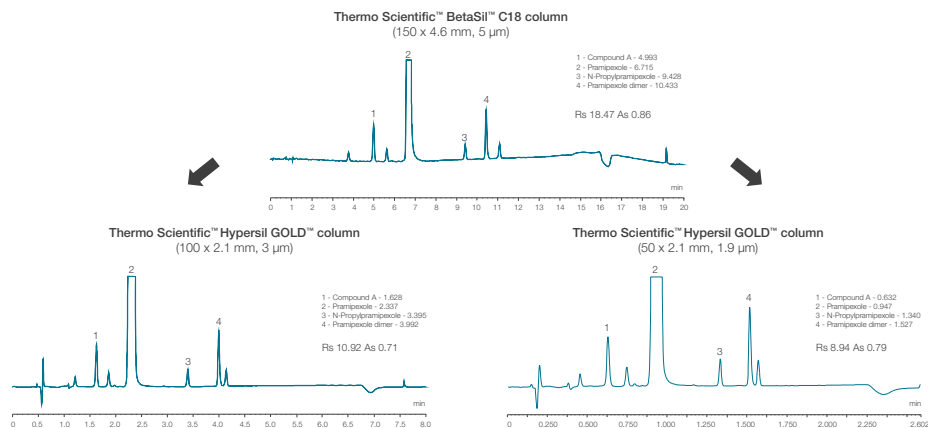

## How to do the calculation

### Moving from original method to improved HPLC technology

#### Calculate new flow

When changing the particle size and ID of your column, you will have to adjust for flow. This is done by this equation:

$$F_2 = F_1 \times \left[ \frac{(dc_2^2 \times dp_1)}{(dc_1^2 \times dp_2)} \right]$$

F<sub>1</sub>= Old flow rate

F<sub>2</sub>= New flowrate

dc<sub>1</sub>= Inner diameter of column originally used

dc<sub>2</sub>= Inner diameter of used column

dp<sub>1</sub>= Particle size used in original method

dp<sub>2</sub>= Particle size used in modernized method

By simply entering in data in the equation we arrive at the new flow. For our selected column for modernization Thermo Scientific Hypersil GOLD C18 column, 3 µm, 100 mm x 2.1 mm ID this will be:

$$F_2 = 1.5 \frac{\text{mL}}{\text{min}} \times \left[ \frac{(2.1 \text{ mm ID}^2 \times 5 \mu\text{m})}{(4.6 \text{ mm ID}^2 \times 3 \mu\text{m})} \right] = 0.52 \text{ mL/min}$$

#### Calculate new gradient

When modernizing your method, it is important to adjust your gradient to the new run time of the method. This way we assure that separation remains as required. This is done by first calculating the new gradient time, t<sub>G2</sub>. Now we have t<sub>G2</sub> we can calculate out new times for our gradient.

$$t_{G2} = t_{G1} \times \left( \frac{F_1}{F_2} \right) \times \left[ \frac{(L_2 \times dc_2^2)}{(L_1 \times dc_1^2)} \right]$$

t<sub>G1</sub> = 1

t<sub>G2</sub>= New gradient time

F<sub>1</sub>= Old flow rate

F<sub>2</sub>= New flowrate

L<sub>1</sub>= Length of column originally used

L<sub>2</sub>= Length of used column

dc<sub>1</sub>= Inner diameter of column originally used

dc<sub>2</sub>= Inner diameter of used column

$$t_{G2} = 1 \times \left( \frac{1.5 \text{ mL/min}}{0.52 \text{ mL/min}} \right) \times \left[ \frac{(100 \text{ mm} \times 2.1 \text{ mm ID}^2)}{(150 \text{ mm} \times 4.6 \text{ mm ID}^2)} \right] = 0.4$$

Table 1. Calculation of new time for gradient

| B,% | Time (min) | Delta t         | New time (min)                                    |
|-----|------------|-----------------|---|
| 40  | 0          | –               | 0   |
| 80  | 15         | 15 - 0 = 15     | Prior time + Delta t x tG2 = 0 + 15 x 0.4 = 6     |
| 40  | 15.1       | 15.1 - 15 = 0.1 | Prior time + Delta t x tG2 = 6 + 0.1 x 0.4 = 6.04 |
| 40  | 20         | 20 - 15.1 = 4.9 | Prior time + Delta t x tG2 = 6.04 + 4.9 x 0.4 = 8 |




# HPLC columns and accessories

Ibuprofen workflow

Cepha antibiotics workflow


## Accucore C18 HPLC columns

Achieve fast, high-resolution separations at low backpressures using Accucore C18 LC columns. Rugged 2.6 µm solid-core particles ensure high efficiencies and enable compatibility with both HPLC and UHPLC platforms. The high bonded phase coverage provides optimal retention of a broad range of nonpolar analytes across multiple applications. Robust bonding technology and automated packing procedures ensure excellent reproducibility and long column lifetimes.

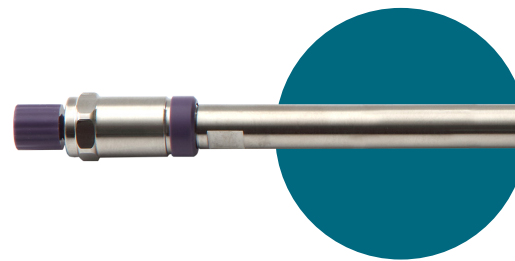

## Hypersil GOLD HPLC columns

Achieve exceptional peak shape and resolution for your HPLC and LC-MS applications with Hypersil GOLD HPLC columns. These endcapped, ultrapure, silica-based columns deliver significant reduction in peak tailing using generic gradients with C18 selectivity. With their excellent resolution, efficiency, and sensitivity, Hypersil GOLD columns give you confidence in the accuracy and quality of your analytical data.

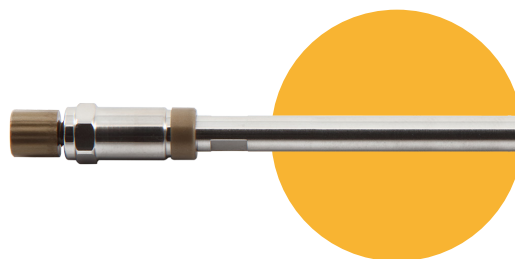

## Uniguard direct-connection guard cartridge holders

Eliminate the requirement for extra fittings using Uniguard direct-connection guard cartridge holders. They are reusable, stainless-steel guard cartridge holders that attach directly to the analytical column inlet.



### Accucore C18 columns

| Format                 | Length (metric) | Particle size | Cat. no.                     |
|------------------------|-----------------|---------------|------------------------------|
| HPLC column            | 100 mm          | 2.6 µm        | <a href="#">17126-104630</a> |
| Guard cartridge (4/pk) | 10 mm           | 2.6 µm        | <a href="#">17126-014005</a> |

### Hypersil GOLD HPLC columns


| Format                 | Length (metric) | Particle size | Cat. no.                     |
|------------------------|-----------------|---------------|------------------------------|
| HPLC column            | 150 mm          | 5 µm          | <a href="#">25005-154630</a> |
| Guard cartridge (4/pk) | 10 mm           | 5 µm          | <a href="#">25005-014001</a> |

### Uniguard guard holder

|   |  |  |                        |
|---|--|--|------------------------|
| Uniguard direct-connection guard cartridge holder |  |  | <a href="#">850-00</a> |
|---|--|--|------------------------|

## Acclaim Polar Advantage II (PA2) HPLC columns

Resolve polar and nonpolar compounds in a single run with Acclaim PA2 reversed-phase columns. These high-efficiency, silica-based columns have a polar-embedded stationary phase that operates over a wider range of chromatographic conditions than possible with conventional reversed-phase stationary phases. Its unique chemistry provides enhanced hydrolytic stability from pH 1.5 to 10 with 100% aqueous mobile phases. The column exhibits selectivity that is complementary to conventional C18 columns and excellent peak shapes for both basic and acidic compounds.

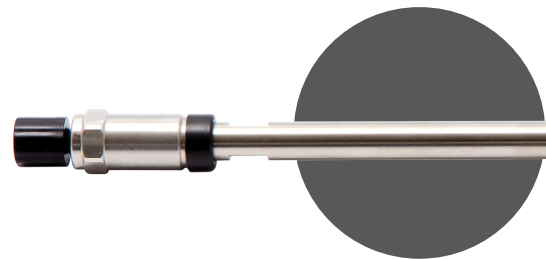

## Acclaim guard holder and coupler



Use the Acclaim guard holder and coupler for your Acclaim guard columns. They can be purchased separately or as a kit.



### Acclaim PA2 columns

| Format   | Length | Particle size | Cat. no.               |
|--|--------|---------------|------------------------|
| HPLC column                                    | 100 mm | 2.2 µm        | <a href="#">068990</a> |
| Guard cartridge (2/pk)                         | 10 mm  | 5 µm          | <a href="#">069692</a> |
| Acclaim guard cartridge holder-coupler kit V-2 |        |               | <a href="#">069707</a> |

## Which Thermo Scientific columns meets your separation needs?

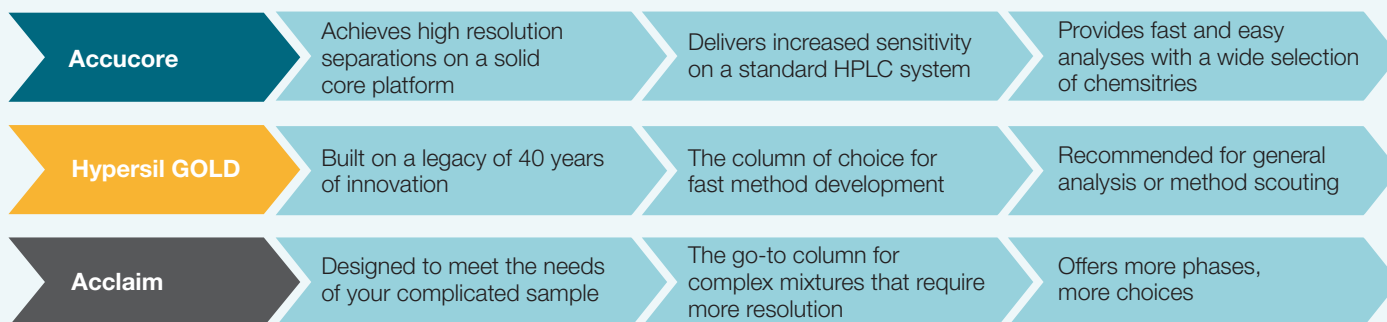

**U/HPLC columns optimized for your analytical performance**

Take a closer look

## TraceGOLD TG-624 and TG-624SiIMS GC columns

Analyze residual solvents, volatile organic compounds, alcohols, and oxygenates using TraceGOLD TG-624 and TG-624SiIMS GC columns. Both phases offer the low to mid polarity phase, 6% cyanopropylphenyl methypolysilozane.



## TraceGOLD TG-WaxMS GC columns

Analyze FAMES with excellent thermal stability using the TraceGOLD TG-WaxMS GC column.

## GuardGOLD guard columns

Protect your analytical column from damage and contamination from nonvolatile materials using the GuardGOLD capillary columns. The columns facilitate superior analytic performance and protect against column contamination caused by nonvolatile materials, extending the column lifetime. The GuardGOLD capillary columns also focus target analytes at the head of the analytical column, leading to better chromatographic peak shape. Highly deactivated to provide superior inertness, essential for analysis of active compounds, and high maximum operating temperature of 360° C.



### TraceGOLD TG-624 and TG-624SiIMS GC columns


| Diameter | Film thickness | Length | Polarity  | Temperature | Cat. no.                   |
|----------|----------------|--------|-----------|-------------|----------------------------|
| 0.32 mm  | 1.8 µm         | 30 m   | Mid-polar | 320° C      | <a href="#">26059-3390</a> |

### TraceGOLD TG-WaxMS GC columns

| Diameter | Film thickness | Length | Polarity  | Temperature | Cat. no.                   |
|----------|----------------|--------|-----------|-------------|----------------------------|
| 0.32 mm  | 0.25 µm        | 30 m   | Mid-polar | 240/260° C  | <a href="#">26088-1430</a> |

### GuardGOLD guard columns

| Diameter | Length | Cat. no.                   |
|----------|--------|----------------------------|
| 0.32 mm  | 5 m    | <a href="#">26050-0532</a> |



**Quality accessories designed to ensure success** [Learn more](#)

## Super Clean gas cartridge filters

Ensure high-purity (99.9999% or 6.0 grade) output gas for optimal GC performance using Super Clean gas cartridge filters. The baseplates can be configured to individual user needs, and there is no contamination during cartridge change. Easy-to-use and cost-effective, Super Clean gas cartridge filters enable fast, tool-free replacement.



## Ferrules and nuts

Use ferrules and nuts to ensure optimal performance. They are available in different materials of various dimension to accommodate a range of instruments, columns and applications.



### Ferrules


| Diameter     | Material      | Size | Cat. no.                 |
|--------------|---------------|------|--------------------------|
| 0.1 to 32 mm | 100% graphite | 10   | <a href="#">290GA139</a> |

### Nuts for capillary GC columns connections

| Diameter      | Material        | Size | Cat. no.                 |
|---------------|-----------------|------|--------------------------|
| Retaining nut | Stainless steel | 5    | <a href="#">35050458</a> |

### Super Clean gas cartridge filters

| Description                                   | Size | Cat. no.                  |
|---|------|---------------------------|
| Gas cartridge filter kit with baseplate       | 1    | <a href="#">60180-830</a> |
| Gas cartridge filter (baseplate not included) | 1    | <a href="#">60180-824</a> |



# Vials and caps

Nitrosamine  
workflow

Ibuprofen  
workflow

Cepha  
antibiotics  
workflow

Solvent  
residue  
workflow

## SureSTART 1.5 mL screw microvials and 9 mm caps

Choose SureSTART 1.5 mL total recovery glass screw top microvials, performance level 3, when you need to maximize the injection volume for <2 mL samples.



## SureSTART 2 mL screw vials

Choose SureSTART 2 mL glass screw top vials, performance level 2, to ensure high quality data with an uninterrupted workflow in high-throughput applications using GC, HPLC/UHPLC, and single or triple quadrupole MS systems.



## SureSTART 20 mL glass screw vials

Use SureSTART 20 mL glass crimp top headspace vials in your highthroughput volatile gas analyses. These headspace vials are made to withstand higher temperatures and internal pressures required for volatile gas analyses.

## SureSTART 9 mm screw caps

Use SureSTART 9 mm screw caps with screw vials that have a 9 mm opening.



## SureSTART 20 mm crimp caps

Use SureSTART 20 mm crimp caps with crimp vials that have a 20 mm opening, including our Thermo Scientific™ SureSTART™ 20 mL glass crimp top headspace vials.



### SureSTART vials

| Type  | Material    | Diameter      | Total volume | Usable volume | Cat. no.                  |
|-------|-------------|---------------|--------------|---------------|---------------------------|
| Screw | Clear glass | 9 mm x 32 mm  | 1.5 mL       | 1.1 mL        | <a href="#">6PSV9-TR1</a> |
| Screw |             |               | 2 mL         | 1.5 mL        | <a href="#">6ASV9-1P</a>  |
| Crimp |             | 20 mm x 75 mm | 20 mL        | 18 mL         | <a href="#">6ACV20-1R</a> |

### SureSTART 9 mm screw caps

| Septum                          | Closure material   | Thickness | Closure size | Cat. no.                 |
|---------------------------------|--------------------|-----------|--------------|--------------------------|
| White silicone/red PTFE/Level 3 | Blue polypropylene | 1 mm      | 9 mm         | <a href="#">6PSC9ST1</a> |
| White silicone/red PTFE/Level 2 | Blue polypropylene | 1 mm      | 9 mm         | <a href="#">6ASC9ST1</a> |

### SureSTART 20 mm crimp cap

| Septum                         | Closure material                   | Thickness | Closure size | Cat. no.                    |
|--------------------------------|------------------------------------|-----------|--------------|-----------------------------|
| Blue silicone/clear PTFE; soft | Red aluminum/<br>magnetic tinplate | 3 mm      | 20 mm        | <a href="#">6PBCC20-ST3</a> |

# Chromatography columns and consumables

Available to order online

**Click. Done!**



A collaboration with Thermo Fisher Scientific gives you the collective power of technology, methods and workflows to serve a wider range of industries and applications – ensuring you and the communities you serve are completely confident in the results.

Ordering your chromatography and analytical science products from us is easier than ever. Once you have set up an online account, simply add your favorite chromatography consumables to your basket, check out online and have your items delivered straight to your door.

## Key features of online ordering

- **24/7** track your order status and view invoices online
- **Check order history** and easily reorder your favorite products
- **Buy** all your Thermo Scientific consumables in one place
- **eProcurement** (B2B) connections available
- **Generate a quote** from the cart, or transfer your cart to colleagues so they can add products, review, or approve the order
- **View** account specific pricing and access web-only price promotions
- **Educational resources** available online with training courses and webinars for your applications



### Workflow solutions for pharmaceutical impurity analysis

Your roadmap on pharma quality control and quality assurance analytical solutions



### Enhance your capabilities

Pharmaceutical applications compendium

Learn more at [thermofisher.com/chromatographyconsumables](https://thermofisher.com/chromatographyconsumables)