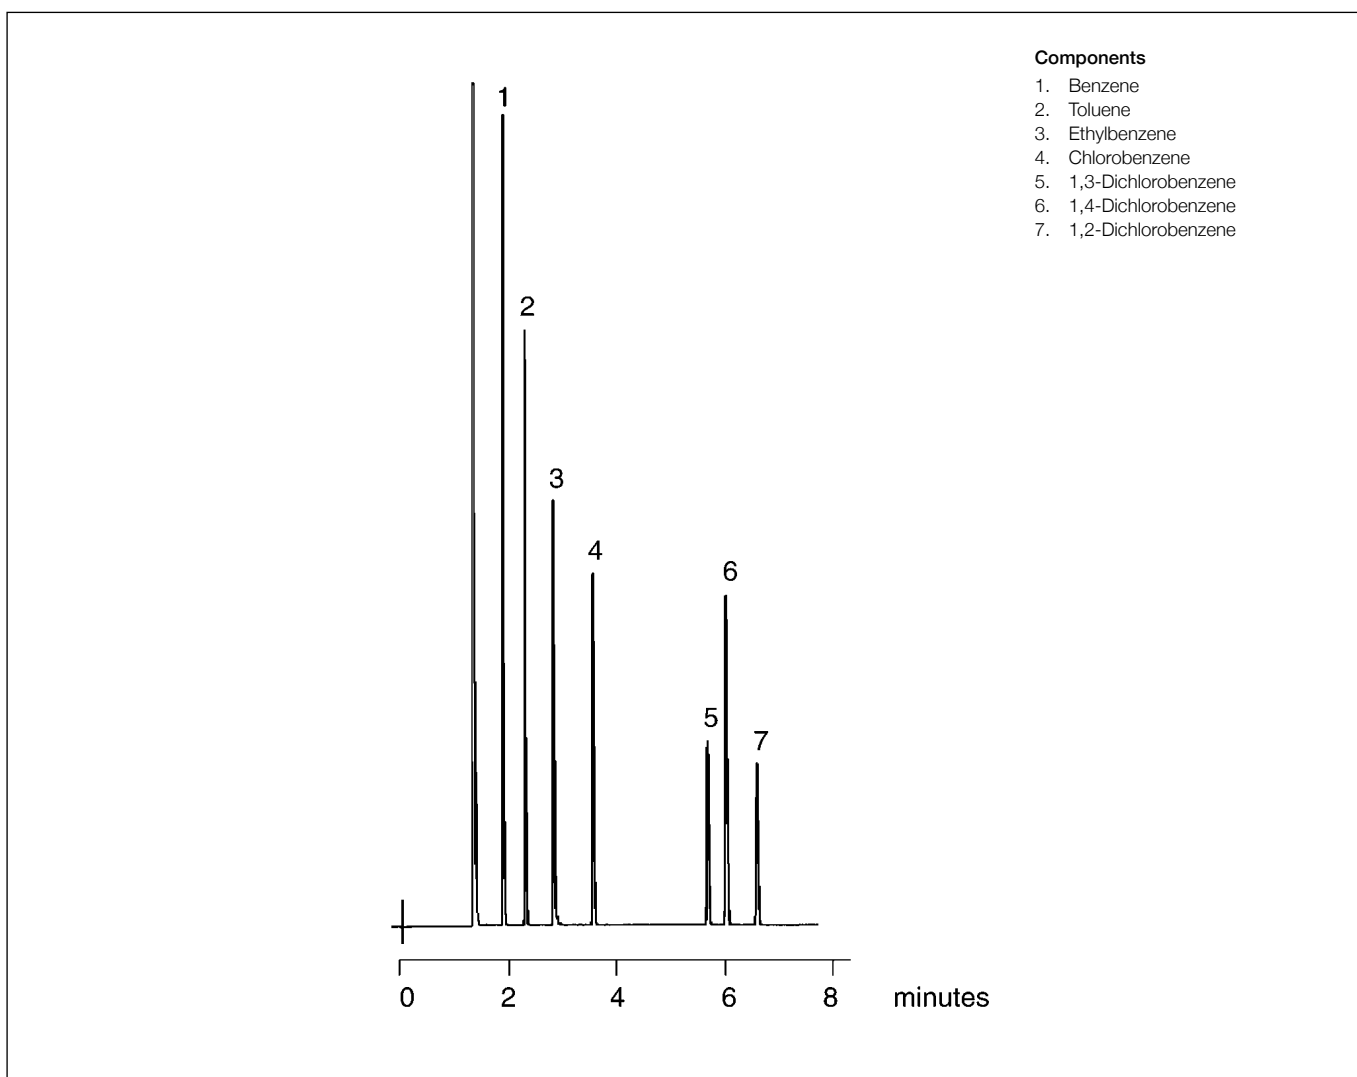


Analysis of aromatics (USEPA 602)

BP20 (WAX)

Column part number	054448		
Phase	BP20 (WAX)	Final temperature	160°C
Column	25 m x 0.53 mm x 1.0 µm	Detector	FID
Initial temperature	80°C, 0 min	Injector	Split
Rate	10°C/min	Carrier gas	H ₂


 For more information visit www.trajanscimed.com or contact techsupport@trajanscimed.com