

# Quantitative clinical toxicological screening comparing Library ID from product ion scan MS/MS to MRM Spectrum mode ID

**ASMS 2017** MP-721

Alan Barnes<sup>1</sup>; Tiphaine Robin<sup>2</sup>; Sylvain Dulaurent<sup>2</sup>;  
Souleiman Elbalkhi<sup>2</sup>; Neil Loftus<sup>1</sup>; Pierre Marquet<sup>2</sup>;  
Franck Saint-Marcoux<sup>2</sup>

<sup>1</sup>Shimadzu, Manchester, UK;

<sup>2</sup>CHU Limoges, Limoges, France.

## Quantitative clinical toxicological screening comparing Library ID from product ion scan MS/MS to MRM Spectrum mode ID

### Introduction

Forensic toxicological sample measurement is commonly performed in a targeted analysis on selected panels of compounds. When using triple quadrupole platforms for analysis, typically two MRMs are used for compound measurement with a quantifier ion transition and reference ion transition. To help reduce false positive and false negative reporting two alternative approaches have been considered; MRM triggered product ion spectrum and MRM Spectrum mode. MRM Spectrum mode

acquires a high number of fragment ion transitions for each target compound generating a fragmentation spectra that could be used in routine library searching and compound verification using reference library match scores.

In this work, we compare different approaches in target quantitation and identification applied to clinical and forensic toxicology.

### Methods and Materials

Whole blood was spiked with a panel of 35 benzodiazepines, or 44 CAO compounds (CAO = cocaine, antipsychotics, amphetamines, opiates), Calibration samples and unknown samples were prepared by QuEChERS method with the inclusion of

stable isotope standards on preparation. Chromatographic conditions were optimized for clinical and forensic toxicology screening and considered the need for rapid polarity switching and chromatographic resolution (Figure 2).

## Quantitative clinical toxicological screening comparing Library ID from product ion scan MS/MS to MRM Spectrum mode ID

Table 1. LC-MS/MS data acquisition conditions.

Liquid chromatography																	
UHPLC	: Nexera LC system																
Analytical column	: Restek Raptor Biphenyl 2.7um 100 x 2.1mm																
Column temp.	: 50°C																
Injection cycle	: 5 µL injection volume																
Flow rate	: 0.3 mL/min																
Solvent A	: Water + 2mM ammonium formate + 0.002% formic acid																
Solvent B	: Methanol + 2mM ammonium formate + 0.002% formic acid																
Binary Gradient	: <table border="1" data-bbox="711 693 1110 998"> <thead> <tr> <th>Time (mins)</th> <th>%B</th> </tr> </thead> <tbody> <tr> <td>1.00</td> <td>5</td> </tr> <tr> <td>2.00</td> <td>40</td> </tr> <tr> <td>10.50</td> <td>100</td> </tr> <tr> <td>13.00</td> <td>100</td> </tr> <tr> <td>13.01</td> <td>5</td> </tr> <tr> <td>17.00</td> <td>Stop</td> </tr> <tr> <td>11-14.2</td> <td>0.5 mL/min</td> </tr> </tbody> </table>	Time (mins)	%B	1.00	5	2.00	40	10.50	100	13.00	100	13.01	5	17.00	Stop	11-14.2	0.5 mL/min
Time (mins)	%B																
1.00	5																
2.00	40																
10.50	100																
13.00	100																
13.01	5																
17.00	Stop																
11-14.2	0.5 mL/min																

Mass spectrometry	
LC-MS/MS	: LCMS-8060
Ionisation mode	: Heated ESI
Scan speed	: 15,000 u/sec
Polarity switching time	: 5 msec
MRM Dwell time	: 2 msec
Pause time	: 3 msec
Interface temp.	: 300°C
Heating block	: 400°C
Desolvation line	: 250°C
Heating gas	: 10 L/min
Drying gas	: 10 L/min
Nebulising gas	: 3 L/min
CID gas pressure	: 250kPa
Interface voltage	: 4 kV

### Spectral Library >1200 compounds

Each library spectrum was acquired using certified reference materials. MRM triggered product ion spectra registered spectra for three collision energies corresponding to CE 10, 35 and 55V as well as a fourth merged CE spectrum totalling 6084 registered spectra. Optimised MRM transitions were determined for all compounds together with retention time.

In this work, MRM Spectrum mode acquired a library of typically 6 MRM's using certified reference materials acquired by LC. The library included not only MRM transitions for each target compound but also retention time (and relative retention time for each internal standard) and meta data including CAS number, formula, synonyms.

# Quantitative clinical toxicological screening comparing Library ID from product ion scan MS/MS to MRM Spectrum mode ID

## Results

### MRM Spectrum mode

To reduce false negative and false positive reporting a higher number of MRM transitions were used for each target compound to increase the level of confidence in assay specificity. The number of fragment ion transitions monitored for each target compound was dependent upon the chemical structure with typically 6 fragment ions for each compound in this work. MRM Spectrum mode combines conventional MRM quantitation with

the generation of a high quality MRM product ion spectrum which can be used in routine library searching and compound verification and identification. A key advantage of using this technique on a fast scanning triple quadrupole mass spectrometer is the capability of library identification without compromising quantitative capability and signal response.

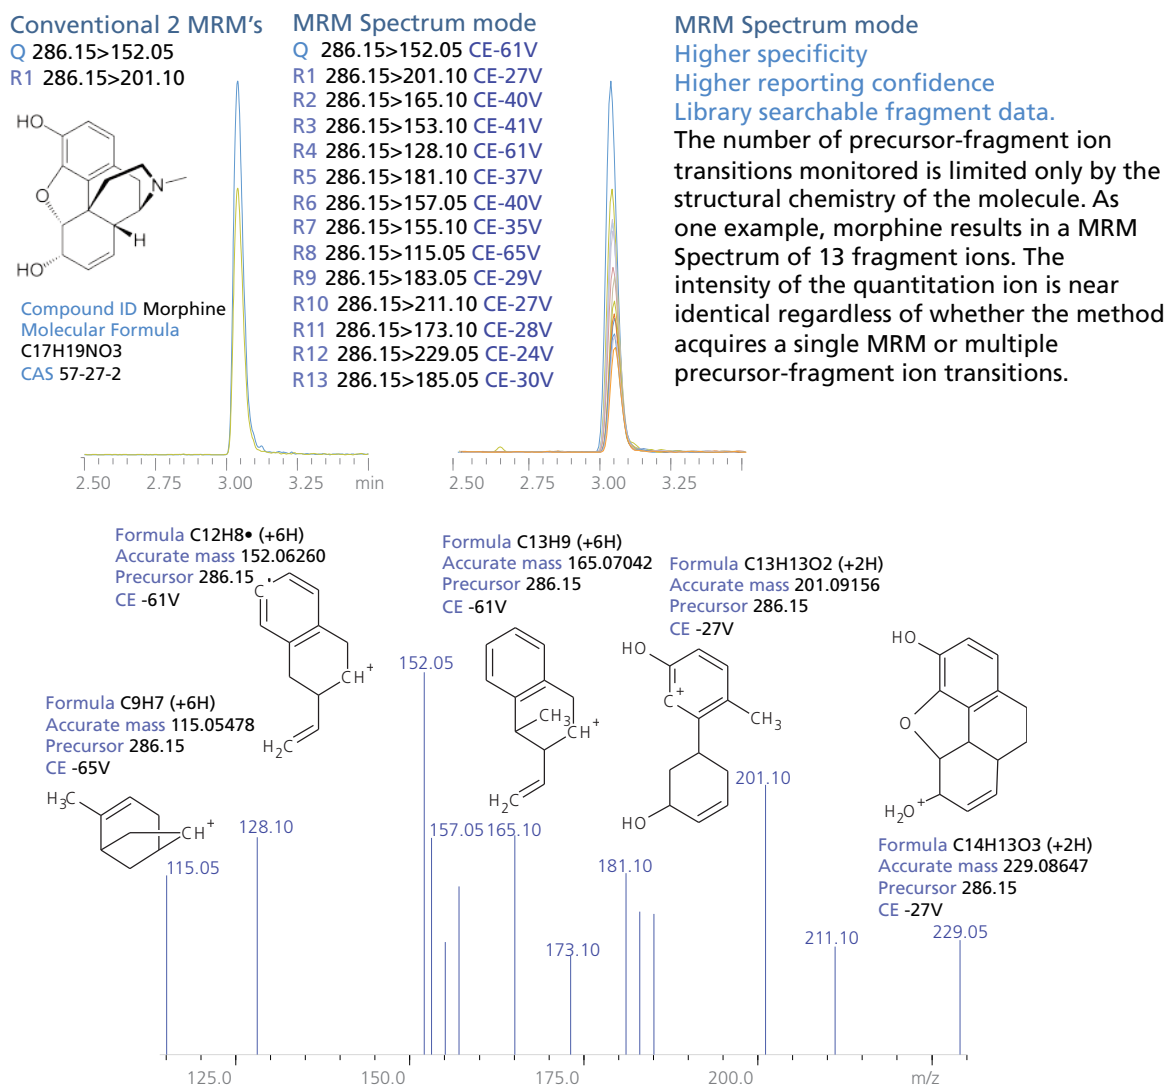


Figure 1. MRM reference spectrum for morphine with putative assigned fragment structures. MRM Spectrum mode combines MRM with the generation of a product ion spectrum. The product ion spectrum can be used for compound identification by searching a library. As the response to each precursor-fragment ion transition has been optimized for a specific collision energy the MRM Spectrum is highly specific and generates strong signal intensities for each fragment ion. (Each precursor-fragment ion transitions structure was assigned using an in house development tool (Structure Analytics) to show commonly described losses and charge migration; the hydrogen deficit is shown in brackets).

## Quantitative clinical toxicological screening comparing Library ID from product ion scan MS/MS to MRM Spectrum mode ID

### Impact on quantitation


To minimize the possibility of false defect reporting without compromising the accuracy, precision and limits of detection, methods were developed to combine the sensitivity of MRM detection with the identification power of a MRM or full scan product ion spectrum. The methods have the capability of simultaneously using both precursor and product ion information enabling precise, accurate quantitation and library searchable compound identification. To assess the impact of methods designed to increase reporting confidence by library searching on quantitation both product ion spectrum methods were compared to a data generated using a conventional 2MRM method. For each target

compound the quantifier ion remains the same but the methods differ in information content and data density.


To test the viability of this approach and to quantify and identify targets in the two test panels, the MRM triggered product ion spectrum acquisition method and MRM Spectrum mode were applied to a series of patient blood samples and compared against a validated LC-MS/MS method using 2 MRM's for each target compound. 44 CAO compounds and 37 benzodiazepines including internal standard compounds were acquired using three different MS/MS methods measured

#### Benzoylcegonine Calibration curve 5-500ug/L

##### Mode 2MRM

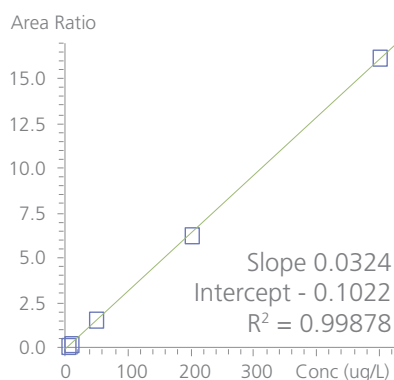

##### Mode MRM Spectrum Mode

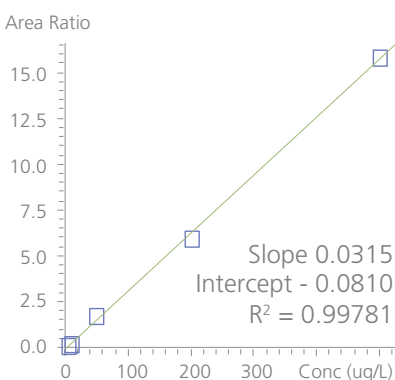

##### Mode MRM triggered product ion spectrum


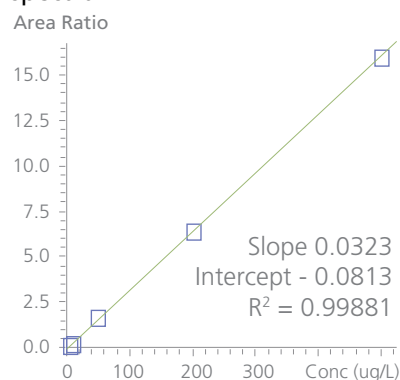



Figure 3. To assess the quantitative impact of both MRM Spectrum mode and a MRM triggered product ion spectrum data acquisition methods, calibration curves were generated over a concentration range of 5-500ug/L spiked into whole blood and extracted with QuEChERS. As one example, the signal response for benzoylcegonine quantifier ion is near identical regardless of the mode of acquisition. (All other compounds in the methods typically achieved  $R^2 > 0.99$ , accuracy 85-115% and precision  $< 10\%$  RSD).

# Quantitative clinical toxicological screening comparing Library ID from product ion scan MS/MS to MRM Spectrum mode ID

Benzoylcegonine QC 50ug/L  
Mode No Library | 2MRM

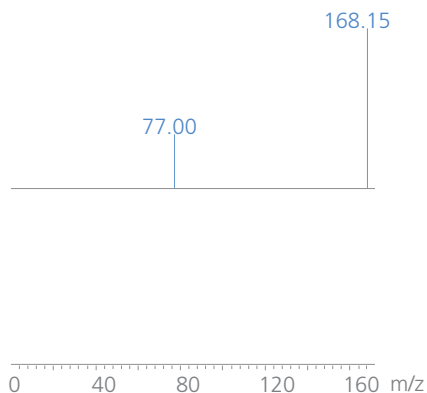

Benzoylcegonine QC 50ug/L  
Similarity Score 99  
Mode MRM Spectrum

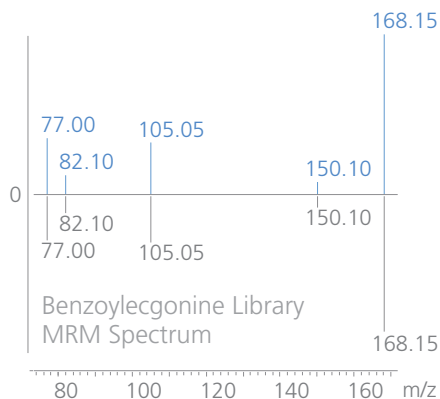

Benzoylcegonine QC 50ug/L  
Similarity Score 78  
Mode MRM triggered  
Product Ion Spectrum

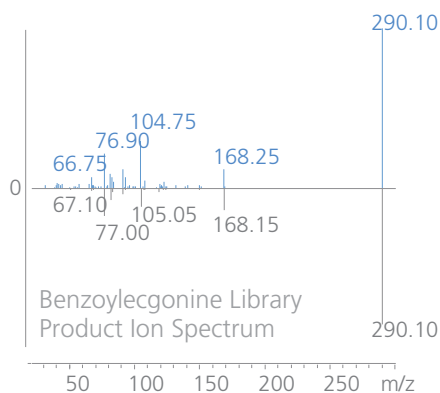


Figure 4. Compared to a conventional 2 MRM data analysis, MRM Spectrum and MRM triggered product ion spectrum data acquisitions deliver library searchable spectra for benzoylcegonine spiked into whole blood at a concentration of 50ug/L.

## Product ion spectrum for increased confidence in compound identification

#	Name	CAS #	Formula	Conc.	R <sup>2</sup>	Found RT
1	Ecgonine methyl ester	7143-09-1	C10H17NO3	77.4	0.9992089	1.035
7	Morphine	57-27-2	C17H19NO3	1321.6	0.9979982	3.312
8	Hydroxymorphone	486-99-9	C17H19NO3	140.8	0.9975141	3.311
18	Resinic acid	1939-41-6	C13H17NO3	126.0	0.9964500	2.190
28	Benzoylcegonine	519-09-5	C16H19NO4	573.5	0.9977332	4.635
42	EDDP	30223-73-5	C20H23N	1458.0	0.9996410	7.514
44	Methadone	76-99-2	C21H27NO	112.0	0.9995477	8.158

#	Lib. #1	Compound Name	RT	CAS #	Formula	URL	Comment	
1	07	Ecgonine methyl ester	1.044	7143	-9-1	C10H17NO3	<a href="http://www.chemspider.com/Chemical-Structure.301036.html?ids:61857b52-bx30-48cc-86c0-7e58a9124059">http://www.chemspider.com/Chemical-Structure.301036.html?ids:61857b52-bx30-48cc-86c0-7e58a9124059</a>	Analgesic, Central Nervous System Agent

## Quantitative clinical toxicological screening comparing Library ID from product ion scan MS/MS to MRM Spectrum mode ID

Figure 5. Using LabSolutions Insight software to review data acquired with unknown patient samples, both MRM triggered product ion spectrum and MRM Spectrum mode deliver the same quantitative data quality compared to a validated conventional 2-3 MRM method.

Compound	Patient Sample – Routine CAO analysis (ug/L)				
	Conventional 2-3 MRM/target	MRM-Spectrum Mode	Library ID# SI	MRM-triggered product ion spectrum	Library ID# SI
	LCMS-8060	LCMS-8060		LCMS-8060	
Benzoylcegonine	>500	>500	99	>500	87
Ecgonine methylester	76.5	77.4	97	80.3	54
EDDP	>500	>500	97	>500	70
Hydromorphone	32.0	31.3	99	39.5	55
Methadone	110.8	112.0	99	111.8	82
Morphine	>500	>500	100	>500	89

## Conclusions

- A generic method was developed for clinical toxicology and forensic analysis using a QuEChERS sample preparation method, a single LC analysis and methods for product ion spectrum identification. By combining MRM quantifier ions with either MRM or scanning product ion scan data both MS/MS method result in higher confidence in compound identification as a result of library searching with robust quantitative data. Library identification added increased confidence to compound identification in situations where reference ion ratios were outside method tolerances or if concentrations measured were below or above LLOQ or ULOQ.
- Both MRM triggered product ion spectrum mode and MRM Spectrum mode generate quantitative data in agreement to a validated conventional MRM method.
- MRM triggered product ion spectrum generates highly rich fragment spectra which has been successfully applied to toxicology.
- MRM Spectrum mode results in high data densities and a high data sampling rate across a peak. This approach generates a consistent loop time and sampling rate producing reliable quantitation and peak integration without threshold triggering and creates new opportunities in screening.

Disclaimer: The Shimadzu LCMS-8060 is intended for Research Use Only (RUO). Not for use in diagnostic procedures. Not available in China.

First Edition: June, 2017